
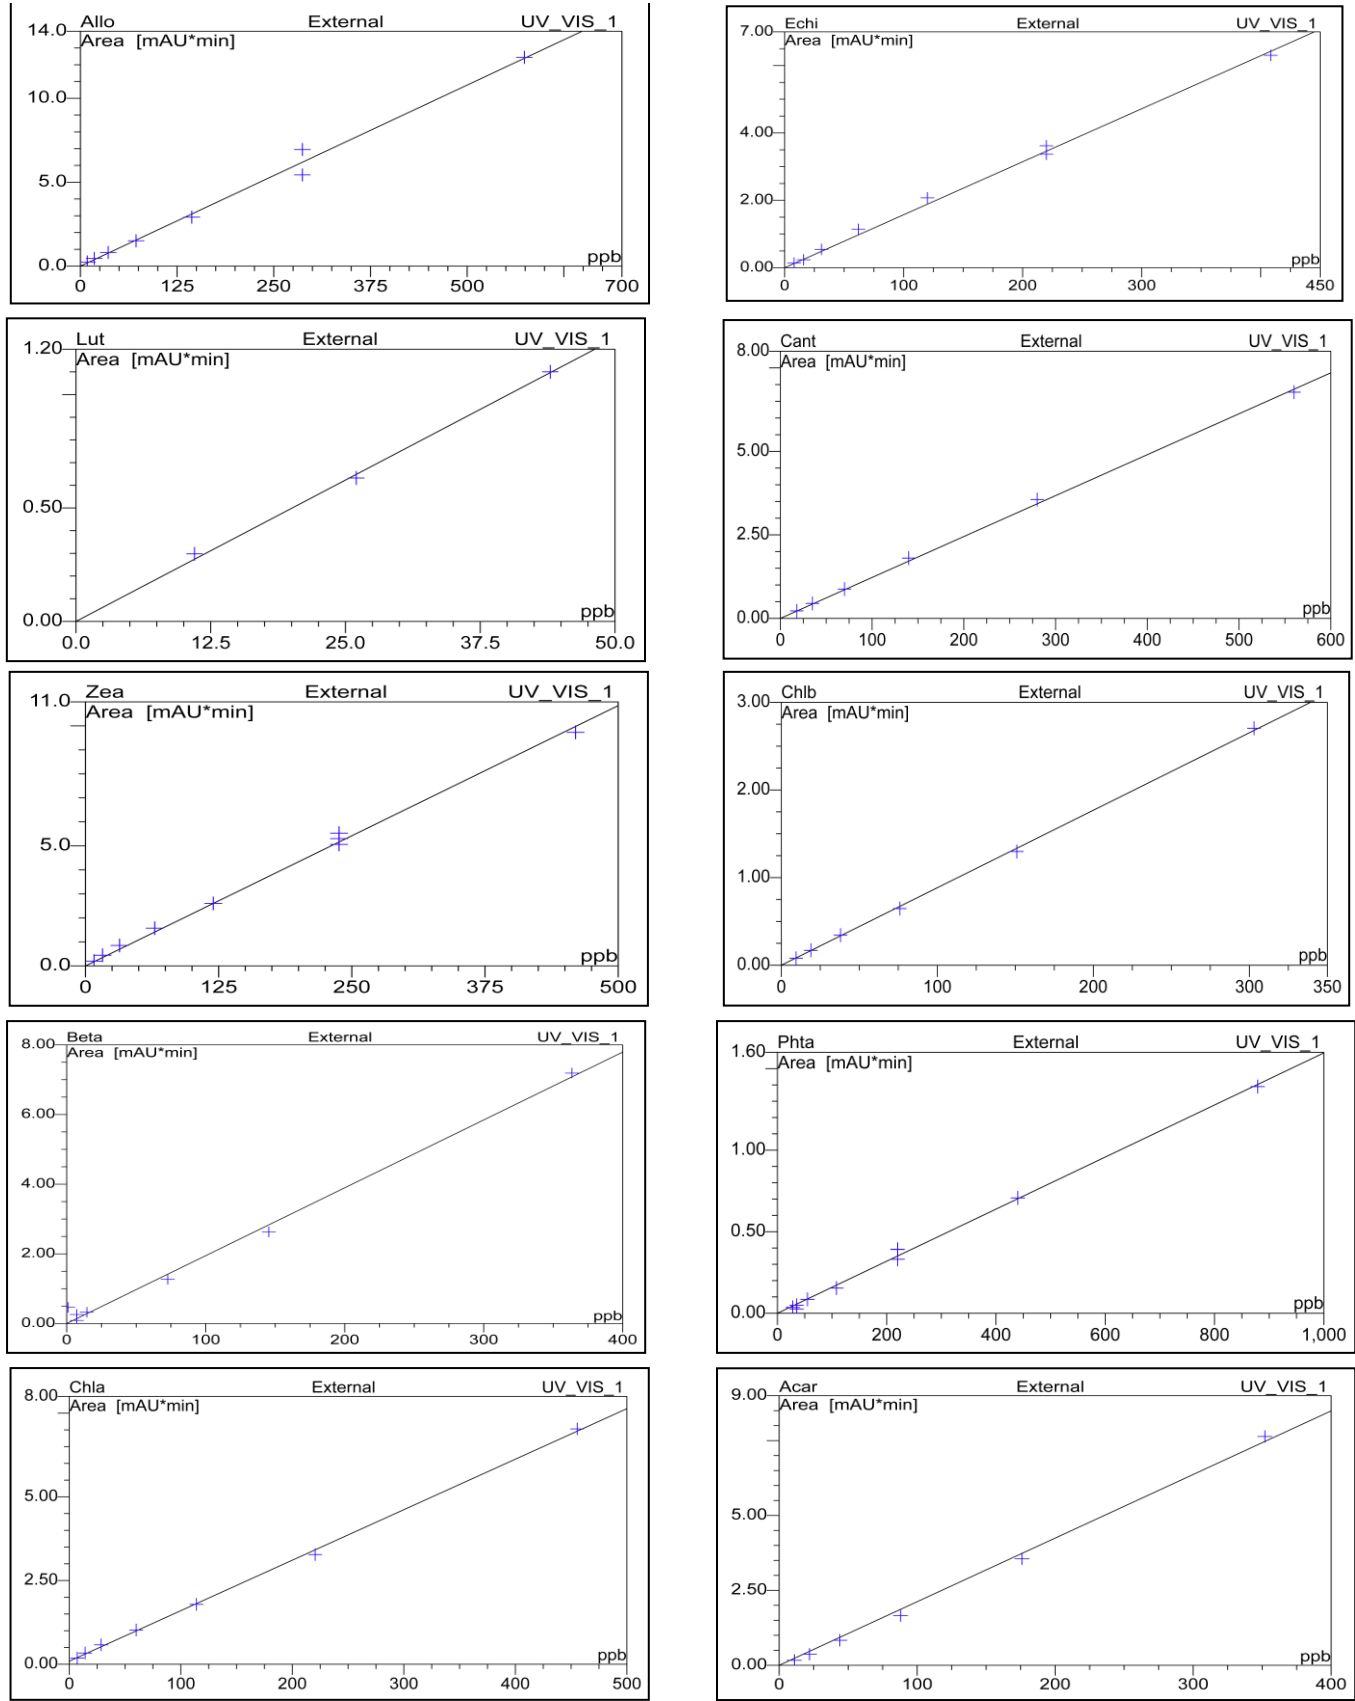


Appendix 11 HPLC Calibration Curves (supplied by AEL)

This Page Left Intentionally Blank

Pigments- Calibration Curves		
Sample Name:	Injection Volume:	350.0
Vial Number:	Channel:	UV_VIS_1
Sample Type: STD	Wavelength:	n.a.
Control Program: PDA Pigments-3Dext	Bandwidth:	n.a.
Quantif. Method: Pigments Quant	Dilution Factor:	1.0000
Recording Time: 29/08/2012 4:01	Sample Weight:	1.0000
Run Time (min): 30.00	Sample Amount:	1.0000

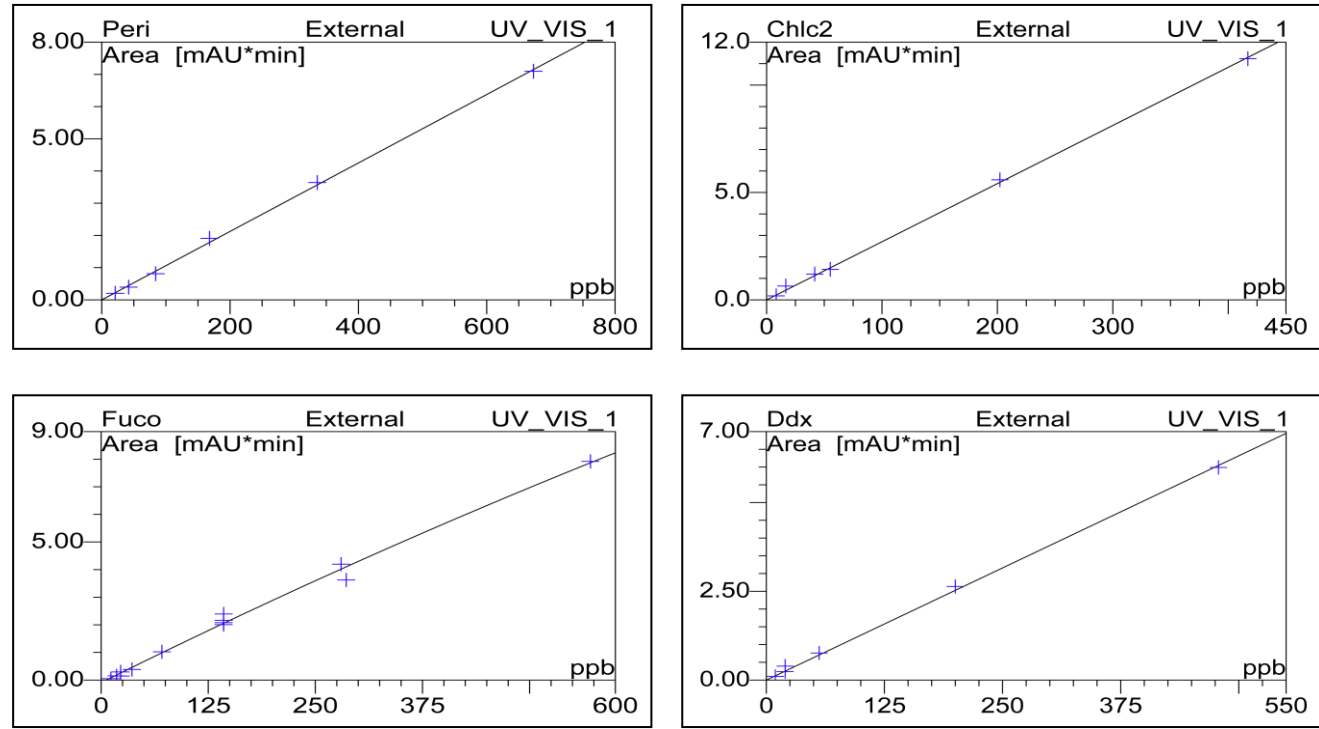

No.	Ret.Time min	Peak Name	Cal.Type	Points	Corr.Coeff. %	Offset	Slope	Curve
1	3.23	Peri	Lin	6	99.9523	0.0000	0.0106	0.0000
2	3.43	Chlc2	Lin	6	99.9709	0.0000	0.0271	0.0000
3	4.89	Fuco	QOff	13	99.5971	-0.0937	0.0154	0.0000
5	6.83	Ddx	Lin	6	99.9501	0.0000	0.0126	0.0000
8	7.65	Allo	Lin	8	99.5207	0.0000	0.0216	0.0000
9	7.99	Zea	Lin	9	99.8774	0.0000	0.0217	0.0000
10	8.25	Lut	Lin	3	99.9058	0.0000	0.0249	0.0000
14	9.79	Cant	Lin	6	99.9627	0.0000	0.0123	0.0000
20	11.01	Chlb	Lin	6	99.9768	0.0000	0.0088	0.0000
22	12.62	Chla	LOff	7	99.9582	0.0905	0.0151	0.0000
23	13.25	DVCh-a	Quad	5	99.7899	0.0000	0.0098	0.0000
24	14.09	Echi	Lin	8	99.8732	0.0000	0.0157	0.0000
27	19.87	Phta	Lin	10	99.8384	0.0000	0.0016	0.0000
29	21.53	Acar	Lin	6	99.9385	0.0000	0.0212	0.0000
Average:					99.8651	-0.0002	0.0156	0.0000

This Page Left Intentionally Blank